

Ordering Information


0.014" Guidewire Diameter

Balloon Diameter (mm)	Balloon Working Length (mm)		
	15	20	40
2.0	620F-15N-31	620F-20N-31	620F-40N-31
2.5	625F-15N-31	625F-20N-31	625F-40N-31
3.0	630F-15N-31	630F-20N-31	630F-40N-31
3.5	635F-15N-31	635F-20N-31	635F-40N-31
4.0	640F-15N-31	640F-20N-31	640F-40N-31

Compliance Chart

Pressure atm (kPa)	Balloon Diameter (mm)				
	2.0	2.5	3.0	3.5	4.0
2 (203)	1.92	2.42	2.89	3.38	3.85
4 (405)	1.96	2.46	2.95	3.44	3.93
NOM* 6 (608)	2.00	2.50	3.00	3.50	4.00
8 (811)	2.04	2.54	3.05	3.56	4.07
10 (1013)	2.08	2.58	3.11	3.62	4.15
12 (1216)	2.12	2.63	3.16	3.68	4.22
RBP** 14 (1419)	2.16	2.67	3.21	3.74	4.30
16 (1621)	2.20	2.71	3.27	3.80	4.37
18 (1824)	2.24	2.75	3.32	3.85	4.45

* Nominal Pressure. The nominal in- vitro device specifications do not take into account any lesion resistance.
** Rated Burst Pressure - Do Not Exceed RBP.

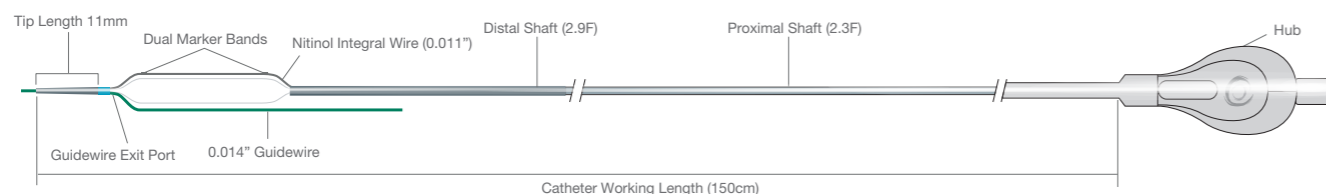

For more information please visit our website at www.OrbusNeich.com or contact us:

EMEA HEADQUARTERS

Drs. W. van Royenstraat 5
3871 AN Hoevelaken
The Netherlands

Phone +31.33.254.1150
Fax +31.33.254.1151

Toll Free Phone 00800.0254.1150*
Toll Free Fax 00800.0254.1151*

* Only for Belgium, Denmark, France, Germany, Ireland, Netherlands, Norway, Sweden and UK

© 2016 OrbusNeich. All rights reserved. **Not available for sale in the USA.**

#G-70-0545 Rev01


Scoreflex and OrbusNeich are registered Trademarks of OrbusNeich Medical, Inc. All data and photos on file. Illustrations are not to be considered as engineering drawings or photos.

Focused Force Angioplasty for the Treatment of Below-The-Knee Arterial Stenosis



Effective Focused Force Dilatation with Dual Wire System

The dual wire system creates a focal stress pattern to facilitate effective controlled plaque modification at low resolution pressure.

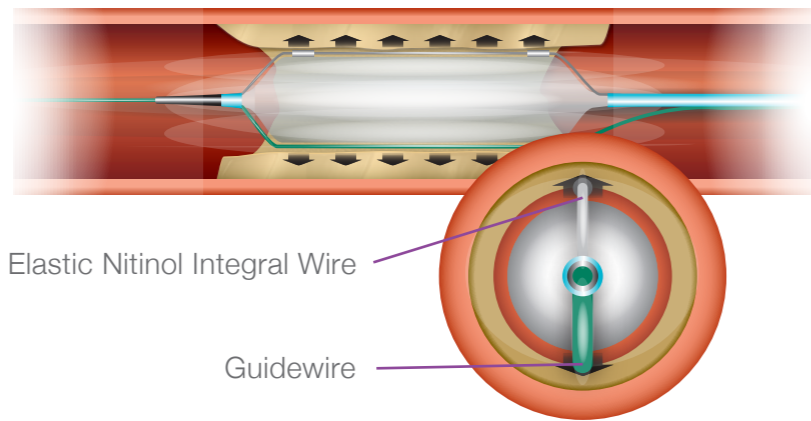

Technical Specifications

Proximal Shaft	2.3F
Distal Shaft	2.9F
Catheter Working Length	150cm
Tip Length	11mm
Guidewire Diameter	0.014"
Nitinol Integral Wire	0.011"
Marker Bands	2
Nominal Pressure	6atm
Rated Burst Pressure	14atm
Coating	Hydro-X (tip & shaft); Invio (balloon)
Minimum Sheath Size	4F

Low Crossing Profile and Unbeatable Trackability

Splendid Crossability

X-Flex tip enables unsurpassed crossability.

Flex Zone

Flexible soft tapered tip allows for smooth lesion entry.

Transit Zone

Transit zone provides a balanced support to guide the balloon to pass through the lesion.

Support Zone

Support zone secures the guide wire exit positioning and assists in pushability of the device.

Tight Fold processing results in a slender primary profile for enhanced crossability through tight lesions.

Soft Balloon Material combined with an elastic nitinol integral wire exhibits exceptional trackability.